

FIG.1

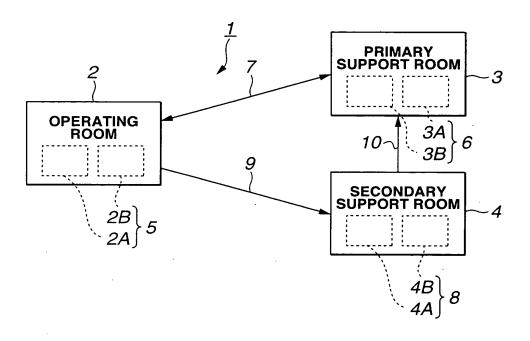


FIG.2




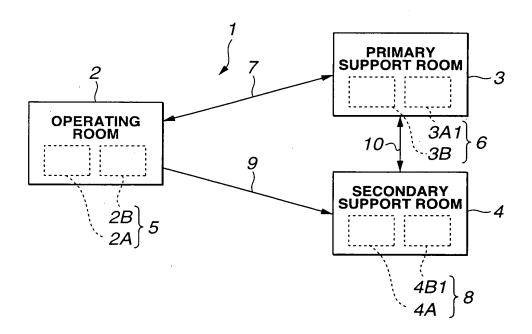


FIG.3

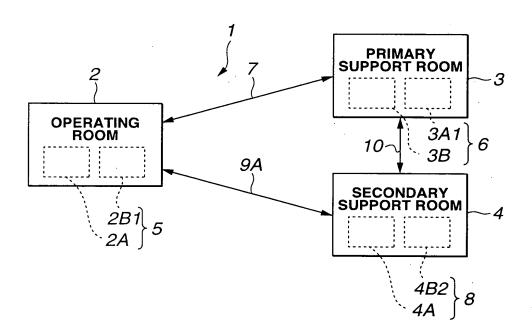

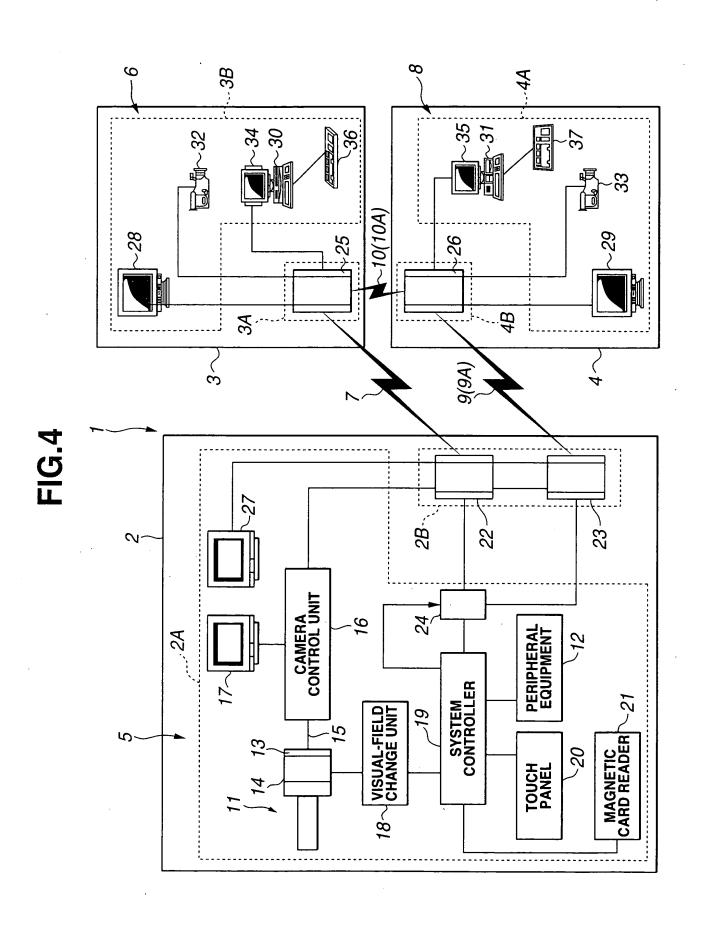

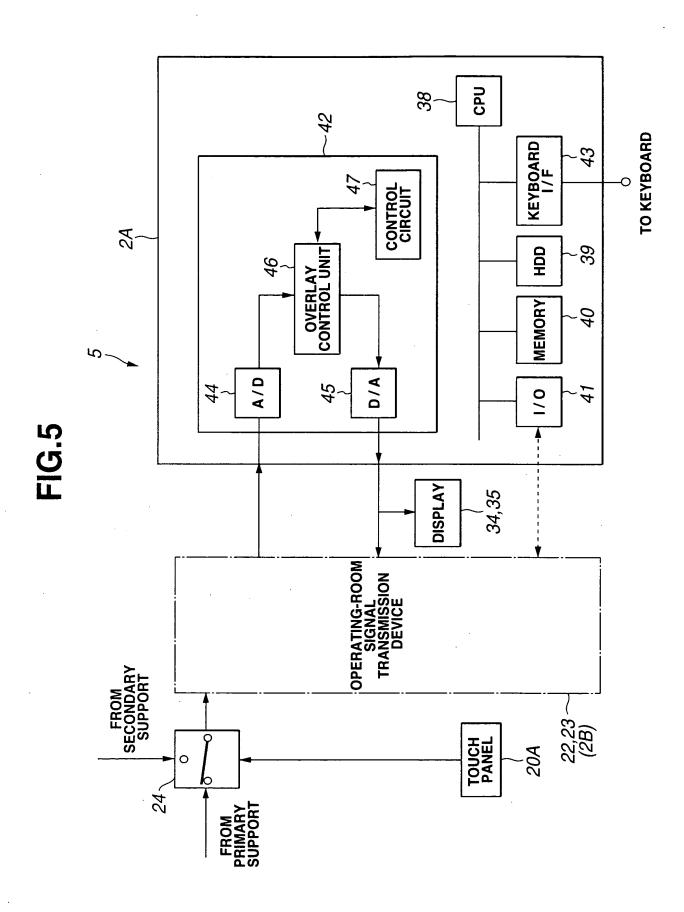

-50 -52 48 NAMESEX FILE NO.DATE OF BIRTHADDRESSMEDICAL HISTORY NO 1 DISPLAY CLEAR 53 INTEGRATED FLOW 162L FLOW HIGH COAGULATION OUTPUT 15W GAS INSUFELATOR FL
SET
PRESSURE PRESSURE
15mmHg 10mmHg
ELECTROCAUTERY
CUTTING COAGULA 8 54 49-51-

**FIG.6** 

## FIG.7

